


Accuratio™ Interpretation Guidelines

CAP™ or Whole PTH™ (pgm/ml)

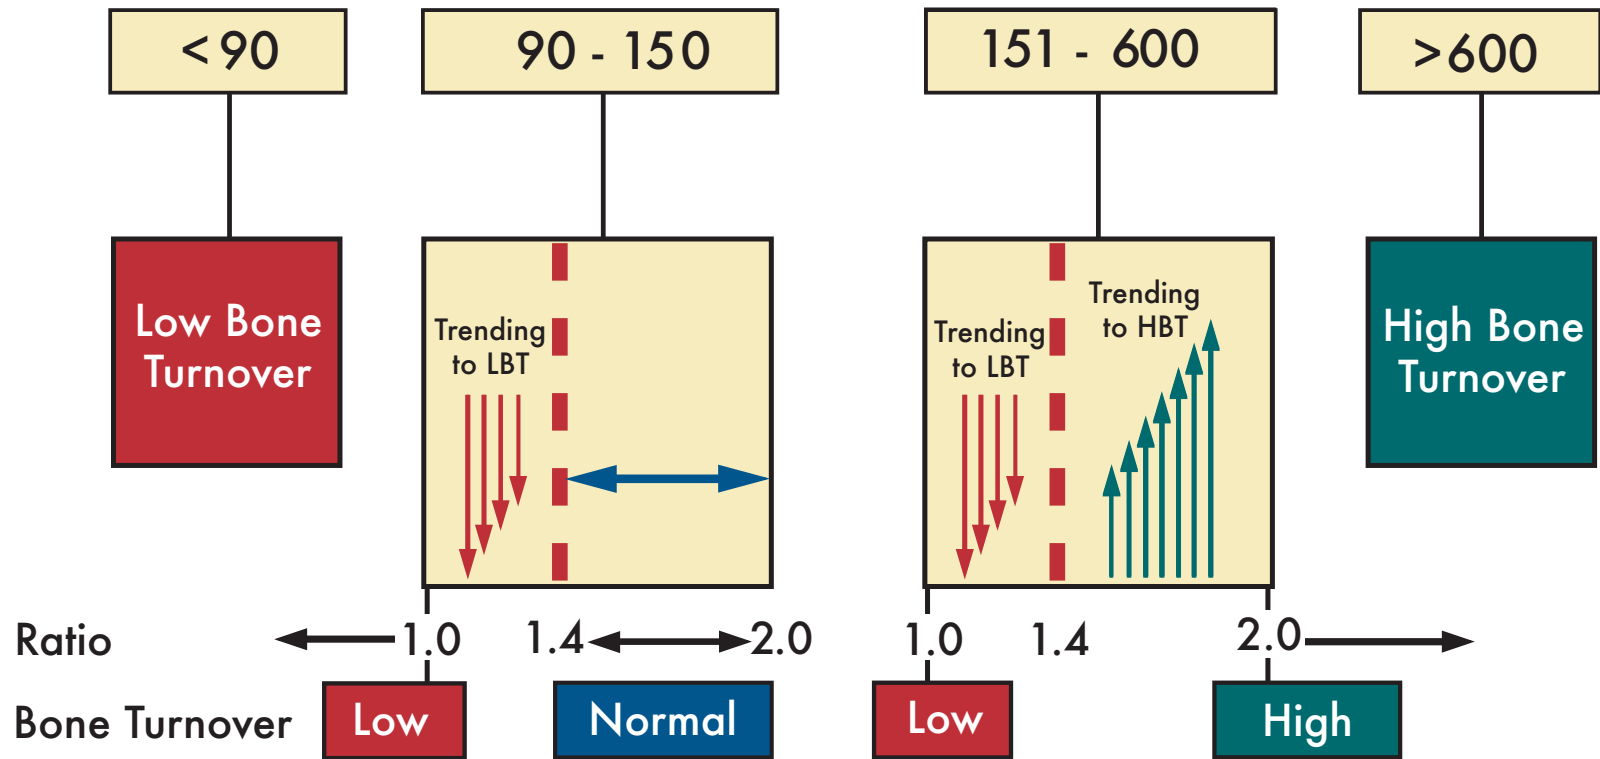

LBT = Low Bone Turnover, HBT = High Bone Turnover. These interpretation guidelines are based on:

- (1) Tokumoto A. *Kidney and Bone Metab* 2004; 17(1):79-86.
- (2) Tokumoto A. Expectation for Whole PTH assay in the dialysis field. *Clin Calcium* 2005; 15(2):273-280.
- (3) K/DOQI Clinical Practice Guidelines for Bone Metabolism and Disease in Chronic Kidney Disease. National Kidney Foundation. *Am J Kidney Dis* 2003(May); 42:S1-S200.
- (4) Faugere M-C, Geng Z, Mawad H, et al. *Kidney Int* 2001; 60:1460-1468.
- (5) Qi Q, et al. *Am J Kidney Dis* 1995; 26:622-631.